

## Certificate of Performance

### TON 2

Product Code KR104

Date 13.03.2020


Expiry Date 13.03.2021

Reagent	Lot Number
TON 1	4350
TON 2	<b>4362</b>
TON 3	4353
Test Method	WC SOP 23
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.001
2.50	TON 100 01 20	0.170
5.00	TON 100 01 20	0.327
7.69	TON 100 01 20	0.495
10.00	TON 100 01 20	0.619

\*serial dilution

### Calibration Curve

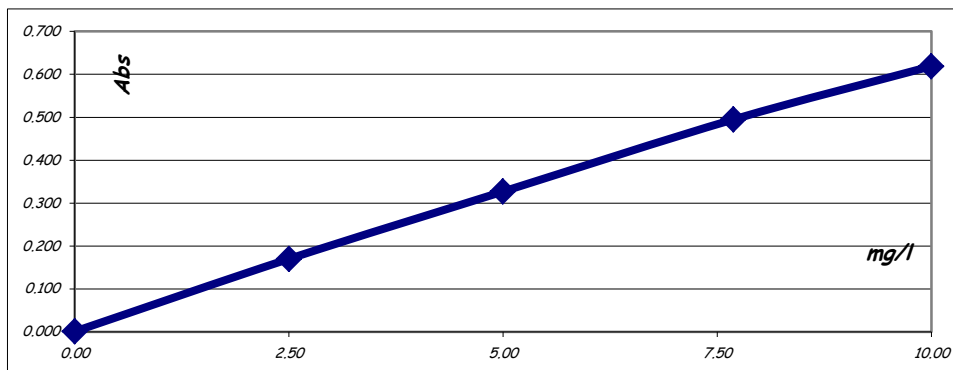

Test	Result	Specification	Pass / Fail
Intercept	0.001	-0.005 to 0.01	Pass
Sensitivity	Abs/ppm		
0 - 2.50 mg/l	0.0676	0.0550 to 0.0800	Pass
2.50 - 5.00 mg/l	0.0628	0.0600 to 0.0800	Pass
5.00 - 7.69 mg/l	0.0625	0.0550 to 0.0800	Pass
7.69 - 10.0 mg/l	0.0537	0.0500 to 0.0700	Pass

Notes

- Store between 2 & 8 °C
- \*Stable on Board TON 1 - 1 day
- \* TON 2 & TON 3 - 5 days
- Keep Tightly Sealed when not in use.
- Do not return unused portions to container
- Barcode ID- TON 1 103; TON 2 104; TON 3 105
- \* Based on results obtained in our Research Facility

*Alan Coonerty*  
A.Coonerty

An ISO 9001:2008 Registered Company  
 Annacotty Business Park, Annacotty, Limerick, Ireland.  
 Telephone 061 358190 Facsimile 061 358191

### Hazard Identification

Labelling according to Regulation (EC) No 1272/2008  
 This reagent is classed as non hazardous.