

## Certificate of Performance

### Ammonia 2 Reagent

Product Code **KR 109**  
 Lot Number **4408**

Date 20.05.2020


Expiry Date 31.03.2021

Reagent	Lot Number
AMM 1	4396
<b>Ammon 2</b>	<b>4408</b>
Test Method	WC SOP 22
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.027
0.25	AMM 10 02 20	0.224
0.50	AMM 10 02 20	0.443
0.77	AMM 10 02 20	0.662
1.00	AMM 10 02 20	0.854

\*serial dilution

### Calibration Curve

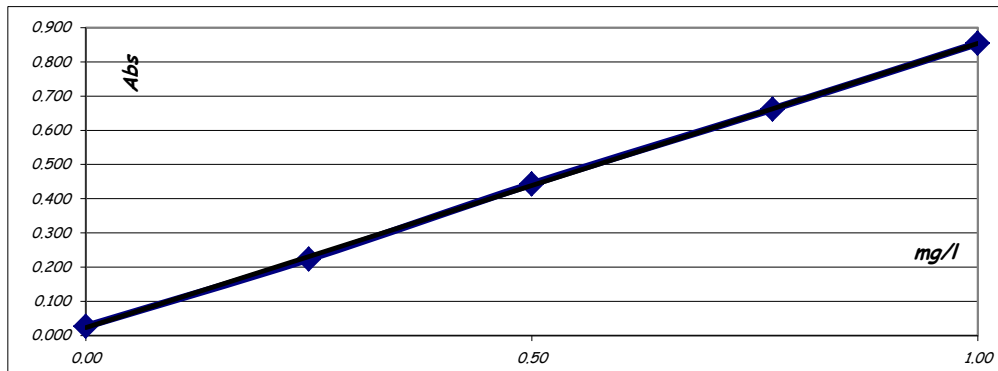

Test	Result	Specification	Pass / Fail
Intercept	0.0236	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.8301	0.750 to 0.890	<b>Pass</b>
Regression	0.9998	0.990 to 1.0001	<b>Pass</b>

Notes  
 Store between 2 & 8 °c  
 \*Stable on Board 5 days  
 Barcode ID = 109  
 \*Based on results obtained in our Research Facility

*Alan Coonerty*  
 A. Coonerty

An ISO 9001:2008 Registered Company  
 Annacotty Business Park, Annacotty, Limerick, Ireland.  
 Telephone 061 358190 Facsimile 061 358191

### Hazard Identification

Labelling according to Regulation (EC) No 1272/2008



Signal Word **Danger**  
**H314** Causes severe skin burns and eye damage  
**H318** Causes severe eye damage  
**H412** Harmful to aquatic life with long lasting effects

Precautionary statements  
 P304+P340  
 P260; P280; P310 P321; P405; P501  
 P303+ P361+ P353  
 P305+P351+P338  
 see full MSDS on [www.serosep.com](http://www.serosep.com)